

5mm-10mm laparoscopes

- I. Base Lever
- II. Positioning Arm
- III. Quick-Mount<sup>™</sup> Lock
- IV. Laparostat<sup>™</sup>
- V. Clamp

- VI. Pin
- VII. Locating Feature
- VIII. Quick-Mount<sup>™</sup>
- IX. Exacting Lever
- X. Rail Adaptor

# Laparostat<sup>™</sup>/Positioning Arm

### INTENDED USE

• The Laparostat holds a laparoscope and attaches into positioning arm.

#### WARNING


- In the U.S.A., federal law restricts device to sale or use by or on order of a physician.
- For illustration purposes only, positioning arm and laparostat may be shown without a cover. Always place a cover over device to protect patients and users from cross-contamination.

Enalish

- Do not use if device appears damaged.
- Positioning Arm Only: Forces exceeding 20lbs. (9.07kg) may move positioning arm when fully locked.
- Do not lubricate device.

### Attaching Positioning Arm and Laparostat \_

- I. Attach positioning arm by turning base handle fully into attachment point.
- 2. Rotate lever to a desired position. Push base handle lever down to secure positioning arm.
- 3. Loosen Quick-Mount lock on positioning arm.
- 4. Insert Laparostat into Quick-Mount, ensuring pin is engaged into locating feature.
- 5. Tighten Quick-Mount lock on positioning arm to secure.
- 6. Place cover over positioning arm and Laparostat, using proper sterile technique (See positioning arm cover instruction).
- 7. Orient positioning arm to desired position. Use exacting lever to tighten arm.
- 8. For initial starting position, center telescoping section of Laparostat and position clamp.

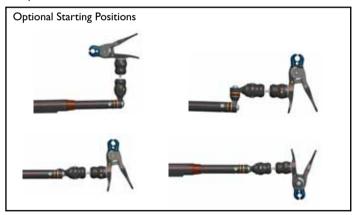

#### NOTE

- Reposition laparoscope by grasping the Laparostat at the clamp.
  - 9. Attach clamp to laparoscope as close to camera body as possible, taking care to avoid puncturing cover. Ensure laparoscope is secure.

### Cleaning and Disinfecting \_\_\_\_\_


WARNING | • Users of this product have an obligation and responsibility to provide the highest degree of infection control to patients, co-workers and themselves. To avoid cross-contamination, follow infection control policies established by your facility.

- - - - -


- Do not place in mechanical washer.
- Do not autoclave or immerse.
- Sterility of positioning arm and Laparostat can only be achieved by using sterile positioning arm cover.
- I. After each use, discard single-use, disposable components.
- 2. Wipe all surfaces with common germicidal or antiseptic wipe, such as alcohol.

## Positioning Arm Cover

# English









- I. Positioning Arm Cover
- II. Quick-Mount<sup>™</sup> attachment opening
- III. Positioning Arm
- IV. Exacting Lever
- V. Attachment
- VI. Quick-Mount
- VII. Quick-Mount Lock